


Broken implant solution with Multi-Unit or Ball Attachment

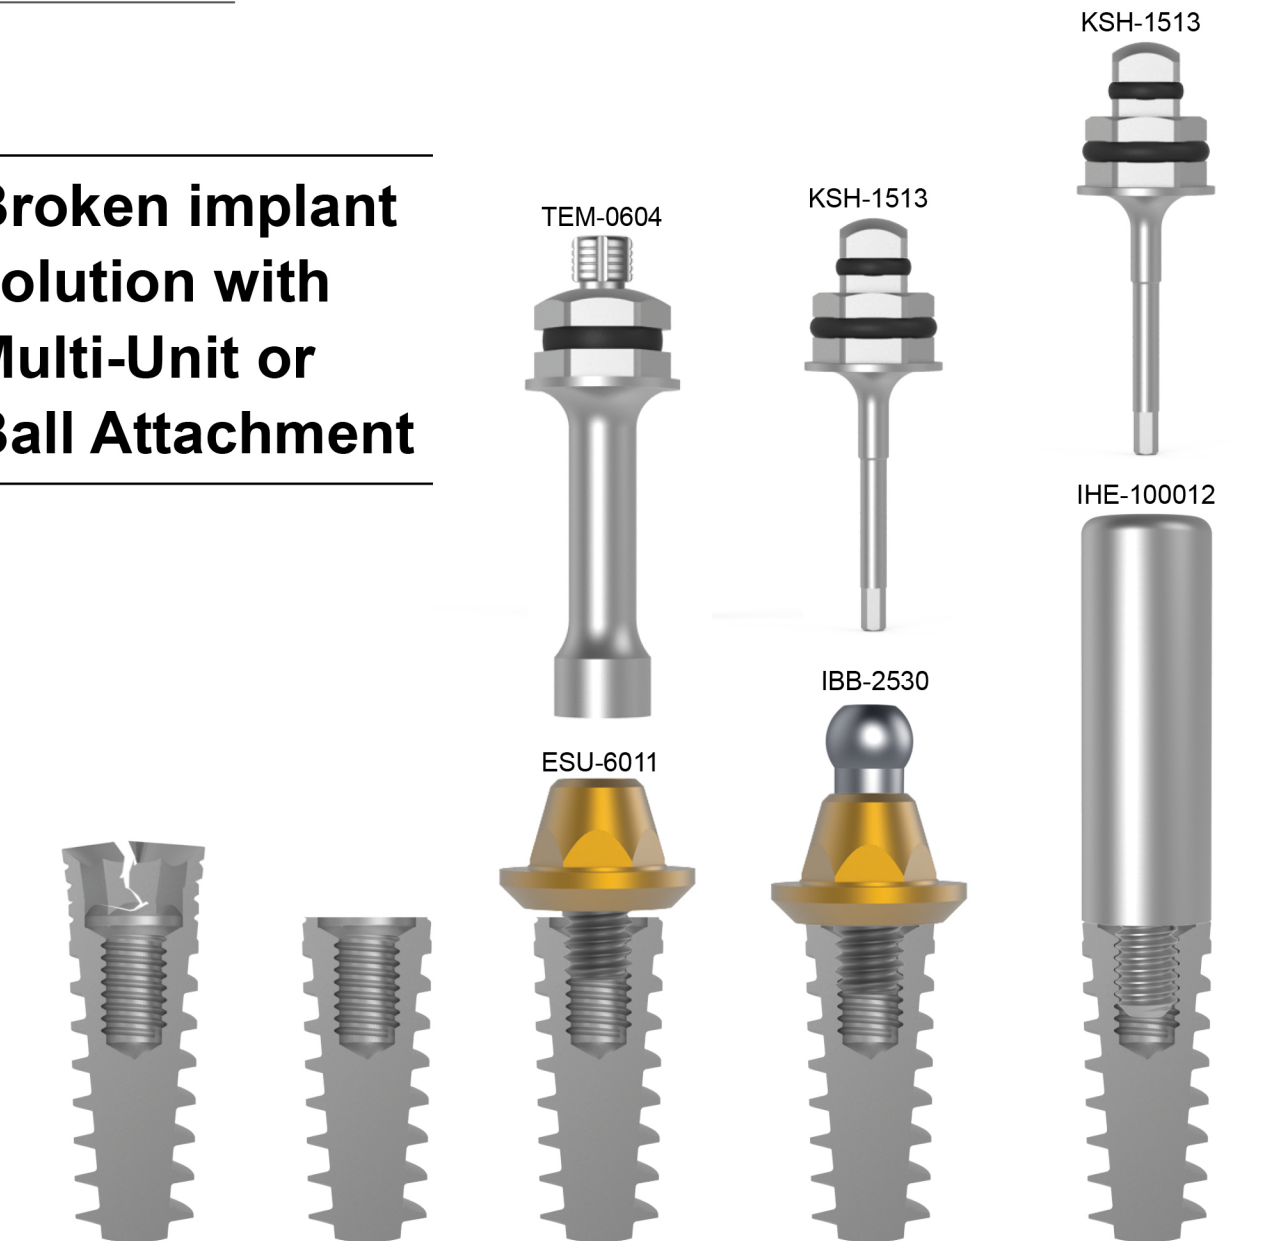

Internal hex broken implant platform

Clean the area from the fractured pieces

Attach the ESU-6011 to the flat with the treads and tighten to 30Nc.

Attach the IBB-2530 to the Multi-Unit and tighten to 15Nc.

Attach the IHE-100012 to the implant and tighten to 30Nc.

Screw retained solution

Over denture solution

Semented solution